


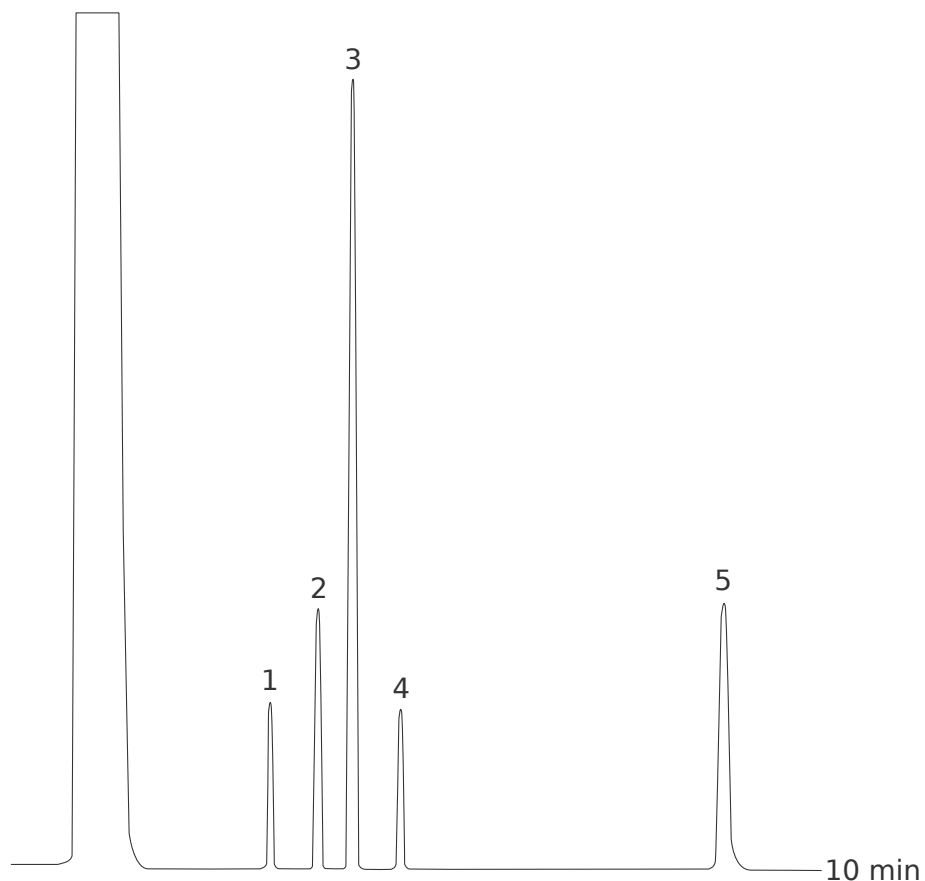

Halogenated Aqueous Compounds

Column: **MEGA-DAI - 0.32mm, 5.00 μ m, 30m**

Catalog Code: C-DAI-032-500-30

MEGA-DAI Column (Direct Aqueous Injections) allows direct introduction of aqueous solutions into the column without sample preparation.

Conditions:

Injection: On-Column.

Detector: ECD 300°C, makeup gas Nitrogen 50mL/min.

Oven Temp.: 104°C Isothermal.

Carrier Gas: Hydrogen, 0.8mL/min.

Peaks:

1. Chlorophorm
2. Methyl-chlorophorm
3. Carbon tetrachloride
4. Trieline
5. Tetrachloroethylene

